

FIGURE 1

FIG. 2 is a perspective view of the device of FIG. 1, showing the device in a retracted position. The device is shown in a retracted position, with the handle 12 and the arm 20 in a retracted position. The device is shown in a retracted position, with the handle 12 and the arm 20 in a retracted position.

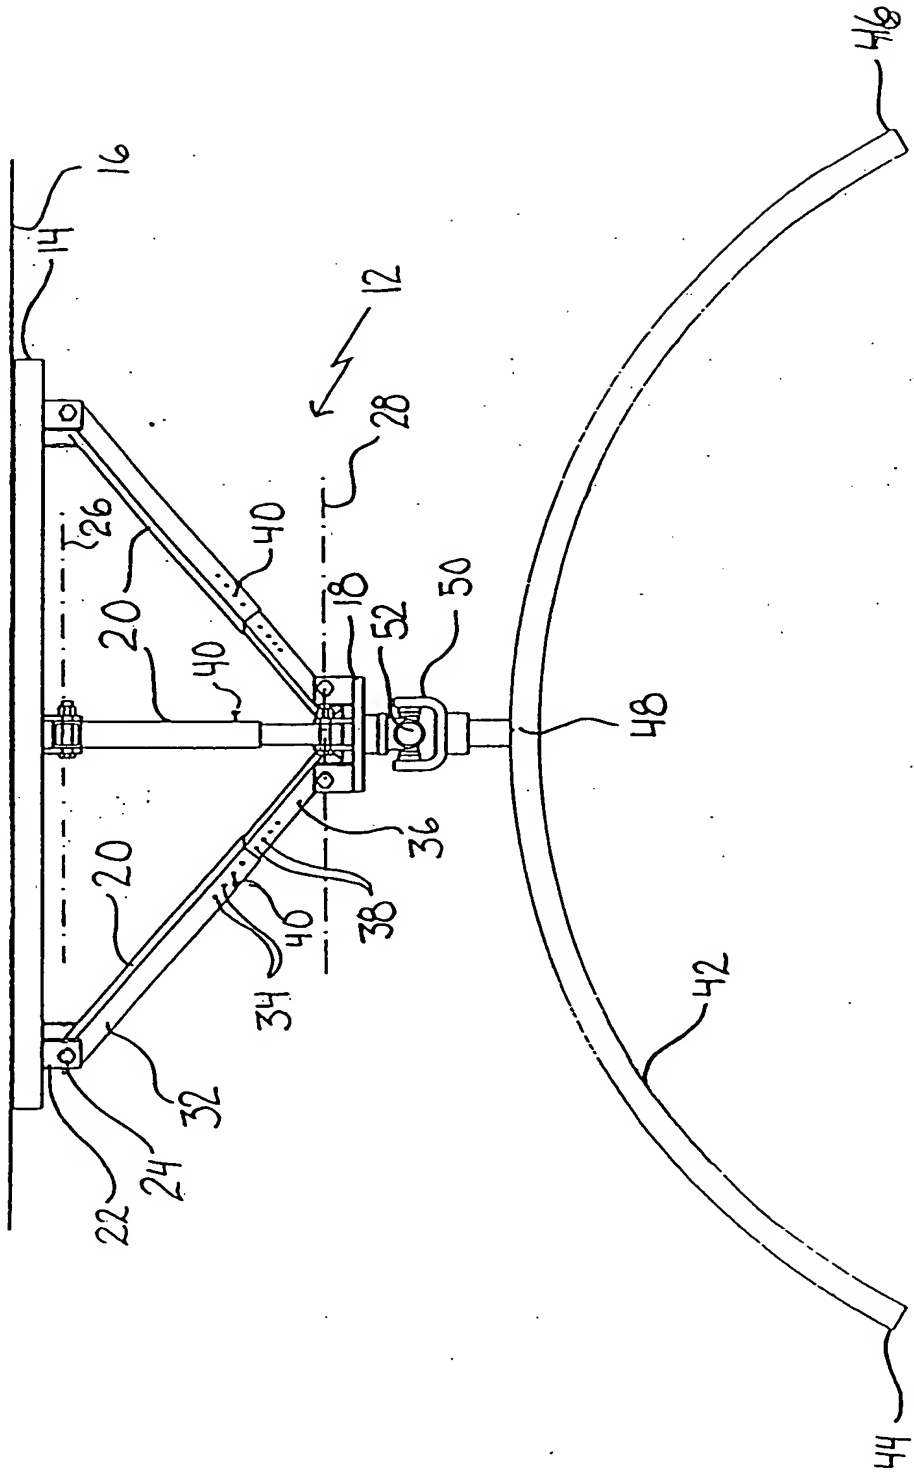


FIGURE 2

FIG. 3

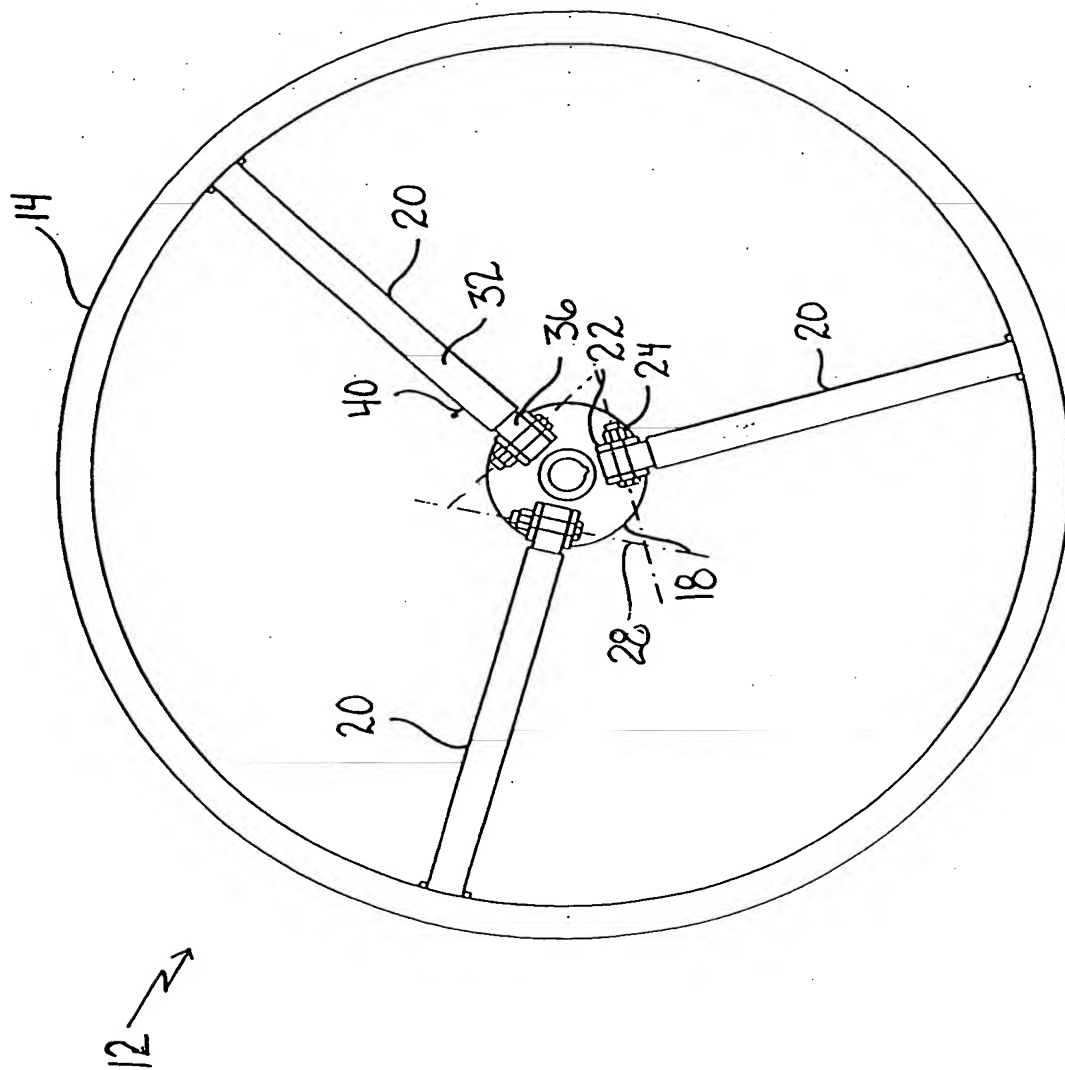


FIGURE 3

2025 RELEASE UNDER E.O. 14176

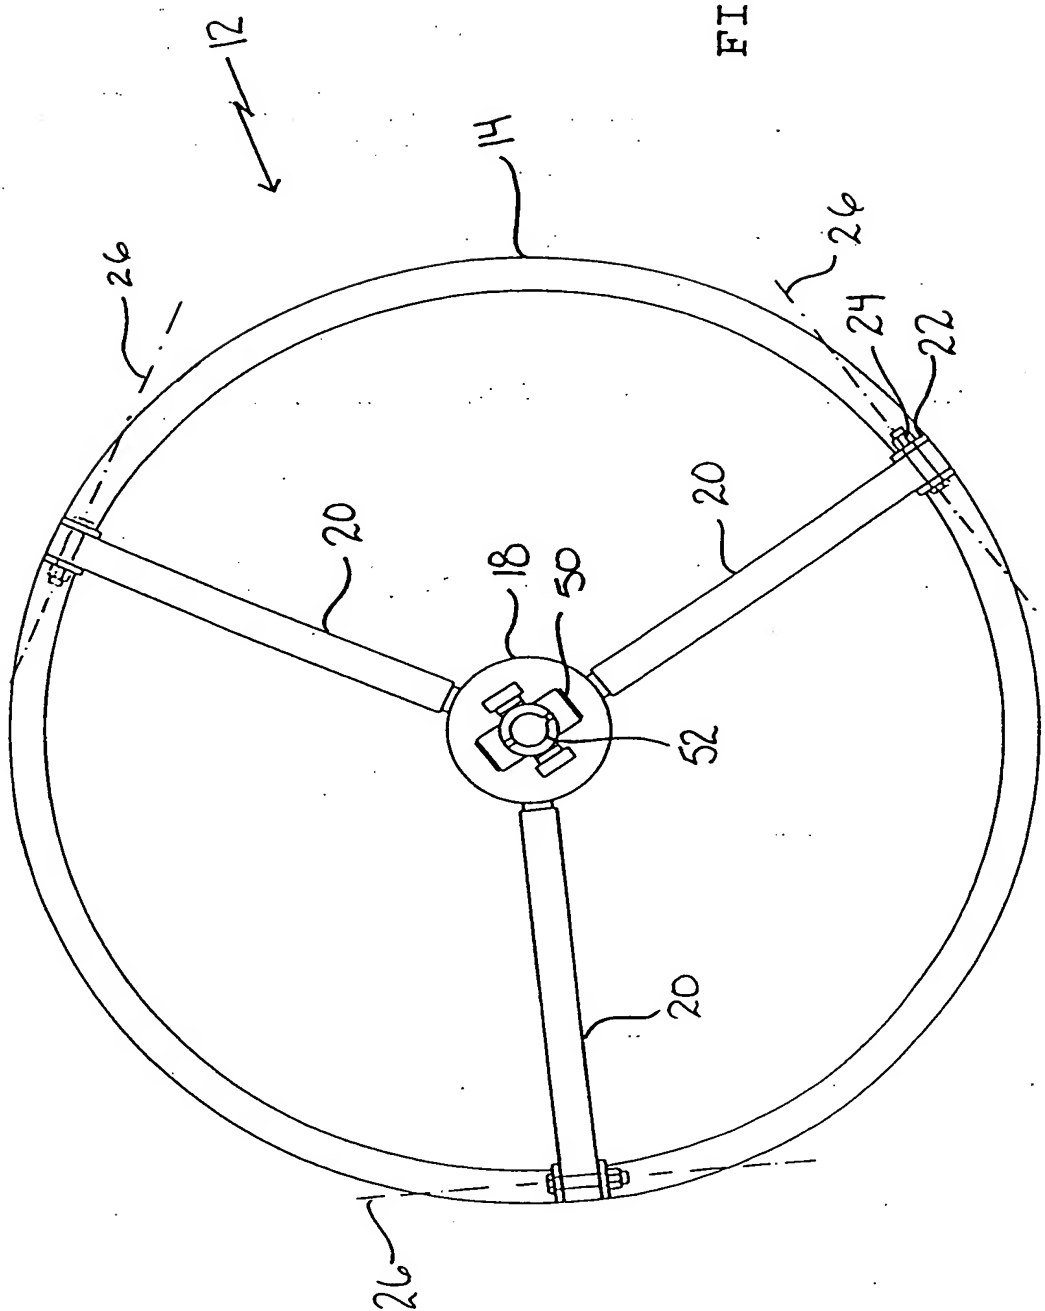


FIGURE 4

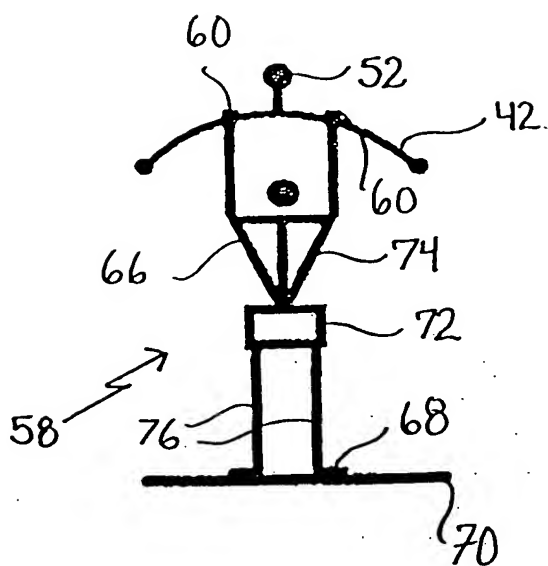


FIGURE 5a

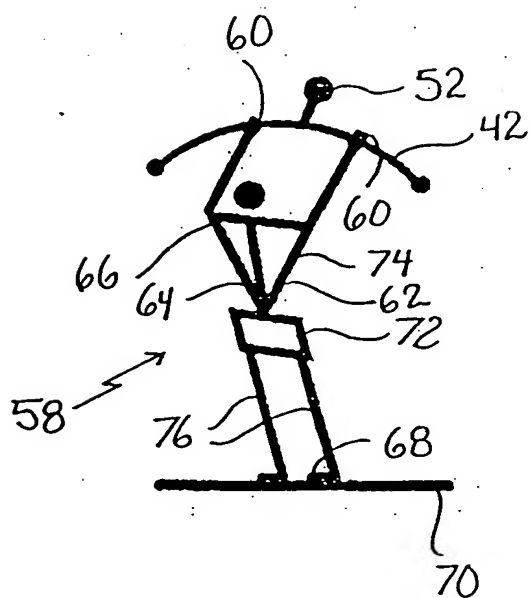


FIGURE 5b

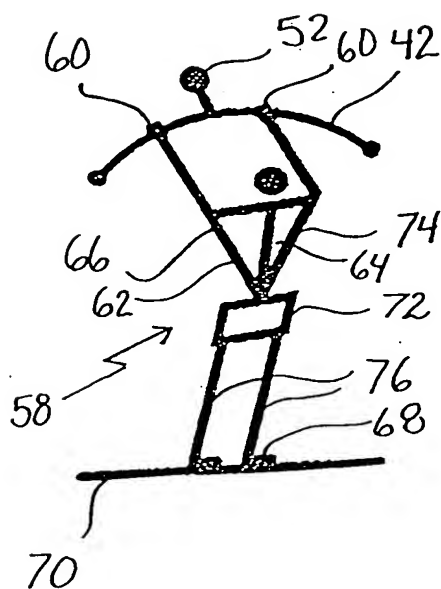


FIGURE 5c

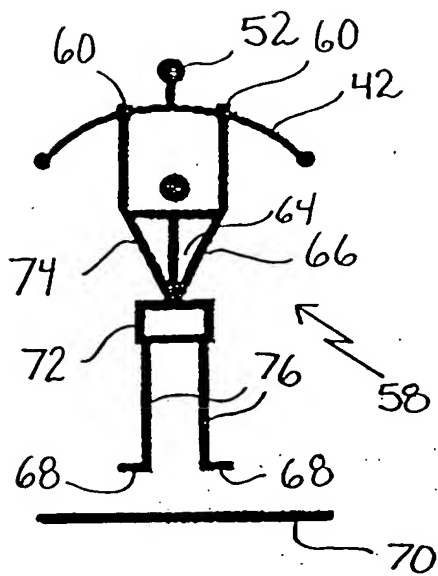


FIGURE 6a

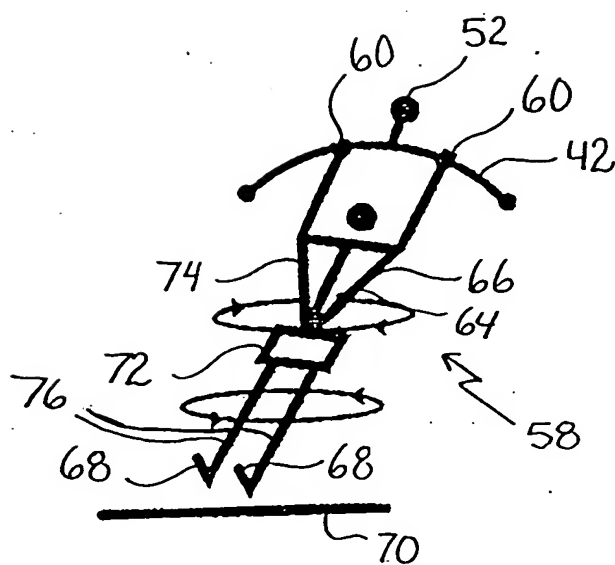


FIGURE 6b

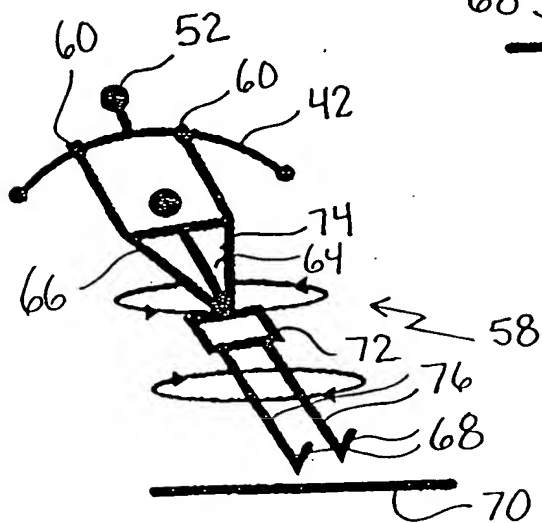


FIGURE 6c

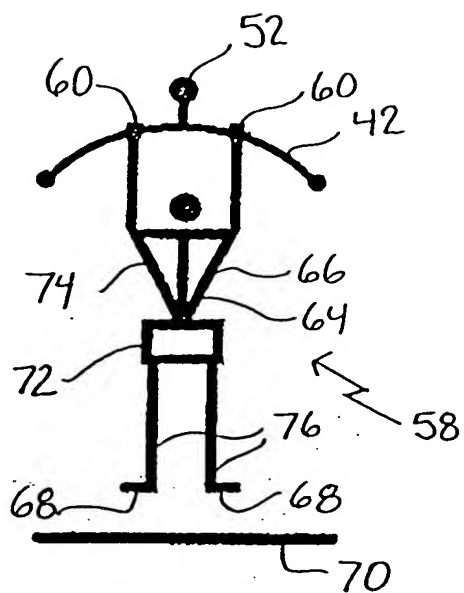


FIGURE 7a

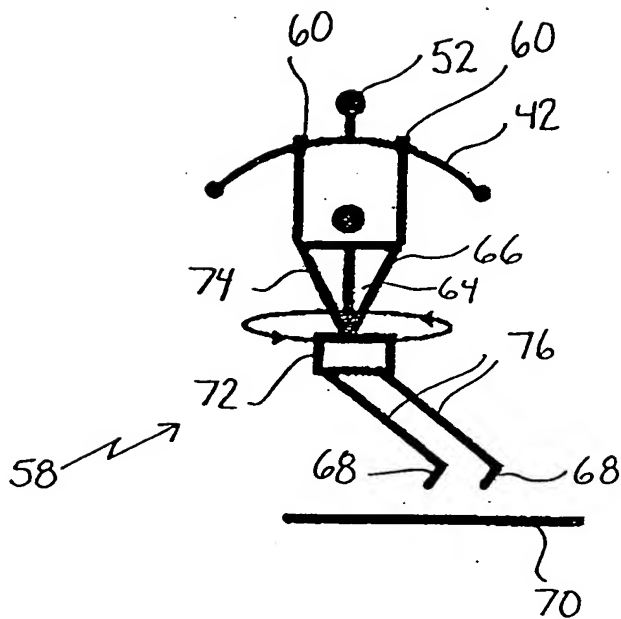


FIGURE 7b

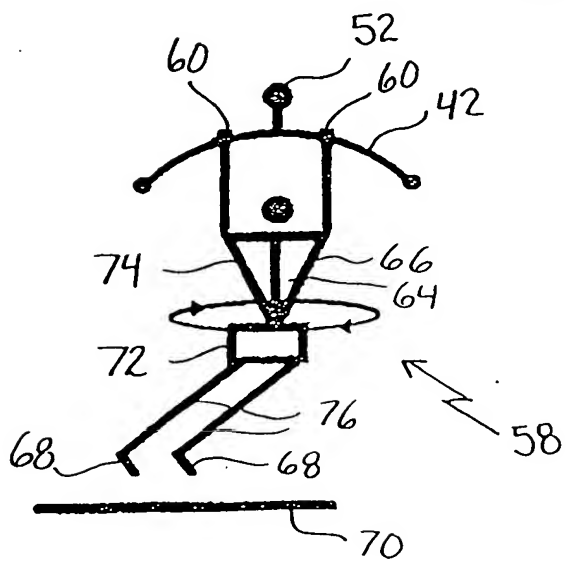


FIGURE 7c